

KinRes: Depth Sensor Noise Reduction in Contactless Respiratory Monitoring

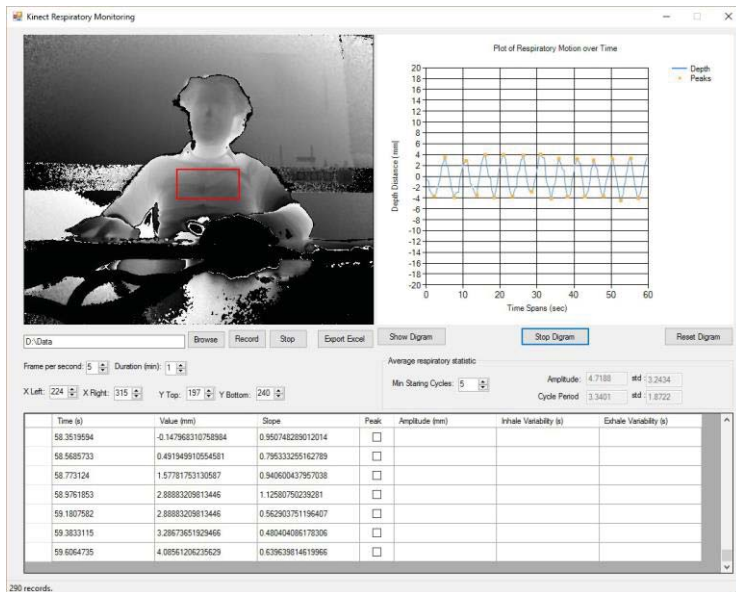


Figure 1: KinRes screenshot with IR 3D Depth image from Microsoft Kinect 2 sensor (left) and the extracted respiratory signal (right).

Kaveh Bakhtiyari
University of Duisburg-Essen
Duisburg, Germany
The National University of Malaysia
(UKM), Bangi, Malaysia
kaveh.bakhtiyari@uni-due.de

Jürgen Ziegler
University of Duisburg-Essen
Duisburg, Germany
juergen.ziegler@uni-due.de

Hafizah Husain
The National University of Malaysia
(UKM), Bangi, Malaysia
hafizahh@ukm.edu.my

Abstract

This paper proposes a novel reliable solution, named KinRes, to extract contactless respiratory signal via an IR-3D Depth sensor (Microsoft Kinect 2) on human subjects interacting with a computer. The depth sensor is very sensitive to the minor changes so that the body movements impose noise in the depth values. Previous studies on contactless respiratory concentrated solely on the still laid subjects on a surface to minimize the possible artifacts. To overcome these limitations, we low-pass filter the extracted signal. Then, a greedy self-correction algorithm is developed to correct the false detected peaks & troughs. The processed signal is validated with a simultaneous signal from a respiratory belt. This framework improved the accuracy of the signal by 24% for the subjects in a normal sitting position.

Author Keywords

Microsoft Kinect; Signal Processing; Greedy Algorithm

ACM Classification Keywords

I.4.3. Image Processing and Computer Vision: Enhancement

Introduction

The human respiratory signal is one of the biological features which is the interest of the researchers in

Permission to make digital or hard copies of all or part of this work for personal or classroom use is granted without fee provided that copies are not made or distributed for profit or commercial advantage and that copies bear this notice and the full citation on the first page. Copyrights for components of this work owned by others than ACM must be honored. Abstracting with credit is permitted. To copy otherwise, or to post on servers or to redistribute to lists, requires prior specific permission and/or a fee. Request permissions from permissions@acm.org.
PervasiveHealth '17, May 23–26, 2017, Barcelona, Spain
© 2017 Association for Computing Machinery.
ACM ISBN 978-1-4503-6363-1/17/05...\$15.00
<https://doi.org/10.1145/3154862.3154896>

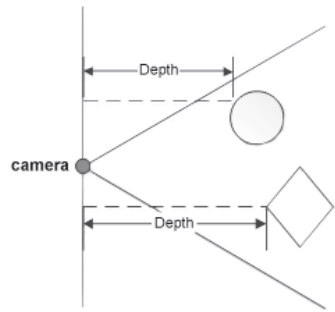


Figure 2: Depth values of the objects within the distance of max 4 meters – Source: “Kinect Sensor: Microsoft Robotics, 2012”

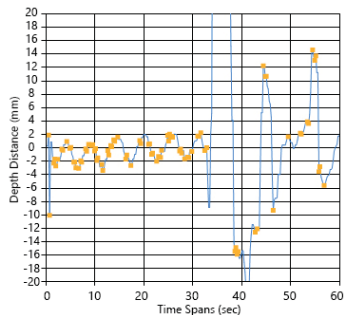


Figure 3: Moving backward and forward interference in respiration monitoring with incorrectly detected peaks and troughs

many areas from medicine [8], rehabilitation [3; 7] and psychology [1] to the computer and cognitive science [2]. Respiratory monitoring devices usually require being attached to the human body in order to acquire the respiration signal, which limits its applications. To overcome this constraint, the contactless respiration monitoring has been suggested with versatile applications. In contactless respiration tracking, a depth sensor is commonly used [4]. Microsoft Kinect 2 is one of the available devices, which is equipped with an IR 3D Depth sensor. As shown in Figure 2, it can measure the object’s depth accurately [5].

To extract the respiration signal from a depth sensor, we need to understand how the human respiratory system works. When a subject is inhaling, the rib cage moves upwards and outwards, and the air is drawn into the lungs. In this case, the chest is getting closer to the sensor, and when exhaling the reverse procedure occurs and the chest would go downwards and backward, and it is getting further from the sensor. Thus, the local minimum in the signal is the inspiration trough and the local maximum is the expiration peak in the respiratory signal from the depth sensor.

Depth sensors are sensitive to the noises, which are generated by: 1) the subject’s movements (Figure 3); 2) data acquisition in a high-frequency sampling rate; and 3) sensor limitations and errors (Figure 5.a). A high quality noise-free signal is essential to measure the respiratory characteristics.

This paper proposes a novel real-time solution, called KinRes¹ (presented in Figure 1), to minimize the error and to maximize the accuracy of the respiratory signal extracted from Microsoft Kinect 2 on a normal sitting user interacting with a computer. To the best of our

¹ KinRes source code is publicly available on [GitHub](#).

knowledge, we are the first to study the subjects’ respiratory signal with normal body movements. KinRes employs signal filters and a smart self-correction method. This system is developed by C#.NET in Microsoft Visual Studio 2015.

Respiratory Signal Characteristics

The respiratory signal in a time domain is the sequential values of the depth changes of the subject’s chest in millimeters. This signal has four main characteristics:

1. *Peak-to-Peak Amplitude* is the depth difference of the two subsequent local maximum (peak) and local minimum (trough), which is in the unit of length.
2. *Inspiration (Inhale) Variability* is the time difference between two subsequent inspiration troughs.
3. *Expiration (Exhale) Variability* is the time difference between two subsequent expiration peaks.
4. *Breaths per Minute (BPM)* is equal to the number of troughs or peaks in one minute.

Methodology

The chest region of interest (ROI) detection is the primary step in signal extraction. This is usually the only area which is being monitored in respiratory tracking systems [4; 9]. Figure 4 illustrates how KinRes operates and is explained as follows.

Noise Filtering

First, the raw signal extracted from the chest ROI is filtered to eliminate high-frequency noise and the native sensor errors by Simple Moving Average (SMA) and Kalman filters (Figure 5.b). After that, the user’s movement would be detected by assigning a moving threshold to differentiate the chest breathing movement from the body movements. The extracted

"Peaks and Troughs" of the respiratory signal are the key elements of the signal characteristics. Peak-Trough Variability (PTV) is proposed as a new self-correction parameter to identify incorrectly measured peaks & troughs."

"KinRes can measure the respiratory characteristics precisely by employing a smart greedy algorithm for self-correction, and decreasing the signal artifacts, noise and errors."

```

PT ∈ [peaks/troughs collection]
for every PTn in PT do
  if PTV(PTn, TTn-1) ≤ 300 ms then
    if f'(PTn) < 0 then
      Remove → min(PTn, PTn-1) ∈ PT
    end if
    if f'(PTn) > 0 then
      Remove → max(PTn, PTn-1) ∈ PT
    end if
  end if
end for

```

Algorithm 1: Abnormal Peak/Trough detection and correction (Self-Correction)

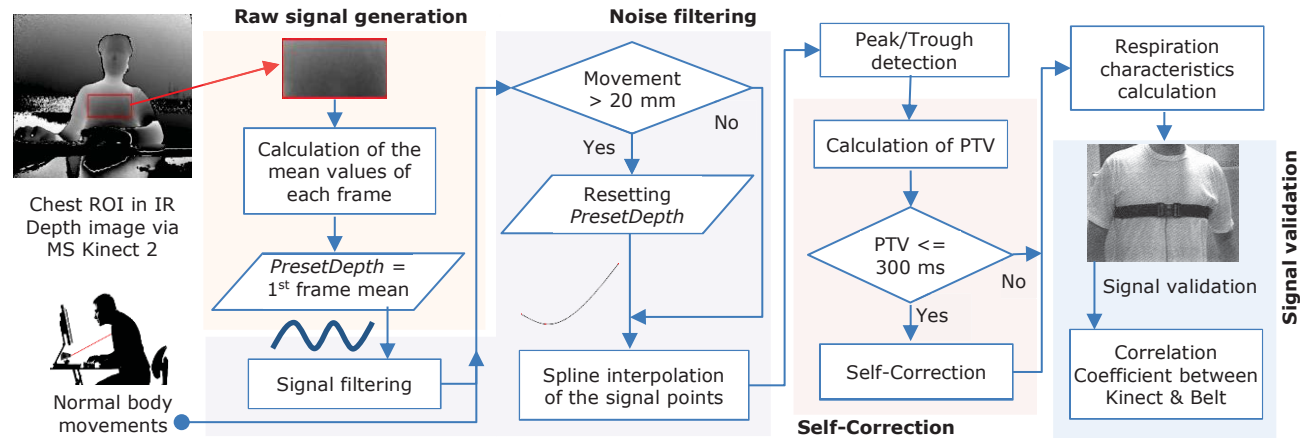


Figure 4: KinRes Methodology: Respiratory signal extraction from an IR Depth sensor (Microsoft Kinect 2)

sampling data are connected with a spline interpolation to generate a smoother signal. When the signal is filtered and interpolated, the peaks and troughs of the signal are calculated to measure the respiratory characteristics.

Self-Correction: Greedy Algorithm

Because of the possible remaining artifacts in the signal, all measured peaks, troughs, amplitudes, and variabilities may be affected. For this purpose, Peak-Trough Variability (PTV) is proposed. PTV is the time difference between two sequential detected peak and trough. Based on the average of all normal PTVs, those out of a threshold band (e.g. 300ms) indicate the incorrectly calculated peak or trough. In the case of abnormal PTV, if the second derivative of the signal was negative, the higher value is accepted as the local maximum, otherwise, in the concave up signal, the lower value is the local minimum (Algorithm 1).

Signal Validation & Results Analysis

In order to evaluate the KinRes signal quality (Figure 6), 24 signals from 12 male subjects (Mean age = 27.58; SD = 2.84) were captured. The process has been performed simultaneously from KinRes (Kinect 2 distance: 1 meter) and the Sleep Sense[®] respiratory belt in a 32 Hz sampling rate for a minimum length of one minute. Then, their correlations were computed. All the signals were acquired in a normal sitting position; however, each participant was recorded in two modes, one with no significant body movements, and the other mode with normal body movements while interacting with a PC.

The best achieved correlation coefficient of KinRes with the Kalman filter on interacting/moving subjects was 0.8637. In overall, the mean correlation coefficient value of 0.9094 of Kalman filter in both modes outperformed SMA (refer to Table 1). Utilized filters improved the accuracy of the system by more than 24% in active mode, compared to the raw depth signal.

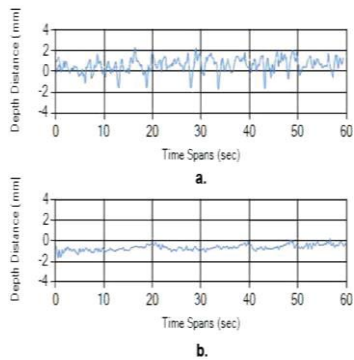


Figure 5: Captured noise from a static object within 60 seconds in the distance of 2 meters from Kinect 2 – a) Raw signal without filtering; b) Filtered signal.

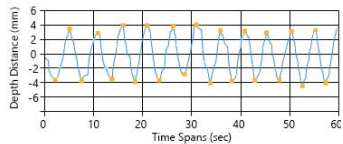


Figure 6: Respiratory signal after noise reduction with correctly detected peaks/troughs

	Static	Active
NO-FILTER	0.8724	0.6195
SMA	0.9565	0.8411
KALMAN	0.9551	0.8637

Table 1: Correlation Coefficient results of two modes of signals (static/still; active/normal) from KinRes against respiratory belt

Despite the higher average correlation of the Kalman filter, it takes few seconds for Kalman to adjust itself with the fluctuations ratio, and the correlation of the signal is lower than SMA at the beginning. However, unlike SMA, it does not require any predefined and fixed frame size.

The result of this study is identical from many aspects in comparison to the prior works. These results are obtained from a normal sitting user behind a desk with normal movements; however, the best-reported results are on the subjects who were laid on a surface similar to the radiotherapy situations [4; 6; 9]. For instance, Xia et al. reported a mean correlation coefficient of 0.969 in a fixed laid position with a translation surface placed on the chest to minimize the noise [9], while this is not a practical position in HCI and pervasive health applications.

Conclusion

This paper has proposed a real-time contactless respiratory tracker, KinRes, which is able to compute and analyze the respiratory characteristics precisely by employing a smart greedy algorithm for self-correction and decreasing the signal artifacts and errors. KinRes was tested on the subjects sitting behind a desk and interacting with a PC; however, the previous studies were done on subjects who were laying down with minimal movements (static). A commercial respiratory belt validated the recorded normalized signals from KinRes, and the correlation results were identically high.

References

1. Alnowami, M., Alnowami, B., Tahavori, F., Copland, M., and Wells, K., 2012. A quantitative assessment of using the Kinect for Xbox360 for respiratory surface

motion tracking. In *SPIE Medical Imaging International Society for Optics and Photonics*, 83161T-83110.

2. Calvo, R.A., D'mello, S., Gratch, J., and Kappas, A., 2014. *The Oxford Handbook of Affective Computing*. Oxford University Press.
3. Chang, C.-Y., Lange, B., Zhang, M., Koenig, S., Requejo, P., Somboon, N., Sawchuk, A.A., and Rizzo, A.A., 2012. Towards pervasive physical rehabilitation using Microsoft Kinect. In *Pervasive Computing Technologies for Healthcare (PervasiveHealth), 2012 6th International Conference on IEEE*, 159-162.
4. Ernst, F. and Saß, P., 2015. Respiratory motion tracking using Microsoft's Kinect v2 camera. In *Current Directions in Biomedical Engineering*, 192.
5. Galna, B., Barry, G., Jackson, D., Mhiripiri, D., Olivier, P., and Rochester, L., 2014. Accuracy of the Microsoft Kinect sensor for measuring movement in people with Parkinson's disease. *Gait & posture* 39, 4, 1062-1068.
6. Lim, S.H., Golkar, E., and Rahni, A.a.A., 2014. Respiratory motion tracking using the kinect camera. In *Biomedical Engineering and Sciences (IECBES), 2014 IEEE Conference on*, 797-800.
7. Mousavi Hondori, H. and Khademi, M., 2014. A review on technical and clinical impact of microsoft kinect on physical therapy and rehabilitation. *Journal of Medical Engineering 2014*.
8. Tahavori, F., Alnowami, M., Jones, J., Elangovan, P., Donovan, E., and Wells, K., 2013. Assessment of Microsoft Kinect technology (Kinect for Xbox and Kinect for Windows) for patient monitoring during external beam radiotherapy. In *Nuclear Science Symposium and Medical Imaging Conference (NSS/MIC), 2013 IEEE*, 1-5.
9. Xia, J. and Siochi, R.A., 2012. A real-time respiratory motion monitoring system using KINECT: Proof of concept. *Medical physics* 39, 5, 2682-2685.